




Instructions for Use

PUREWICK™

FEMALE EXTERNAL CATHETER



Setup:

1. Connect the canister to wall suction and set to a minimum of 40mmHg continuous suction. Always use the minimum amount of suction necessary. If using the DRYDOC™ Vacuum Station, connect the canister to the unit and turn the unit on. Please consult the DRYDOC™ Vacuum Station User Guide for further information.
2. Using standard suction tubing, connect the PUREWICK™ Female External Catheter to the collection canister.

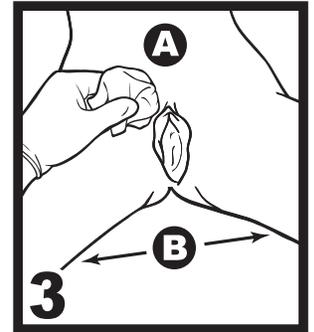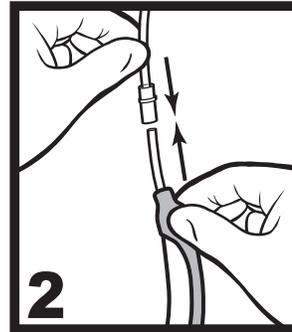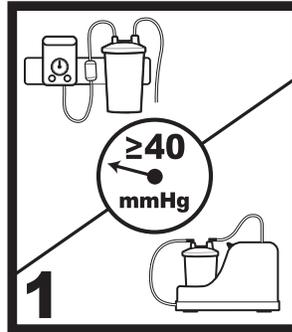

Peri-care and Placement:

3. Perform perineal care and assess skin integrity (document per hospital protocol). Separate legs, gluteus muscles, and labia. Palpate pubic bone as anatomical marker.
4. With soft gauze side facing patient, align distal end of the PUREWICK™ Female External Catheter at gluteal cleft. Gently tuck soft gauze side between separated gluteus and labia. Ensure that the top of the gauze is aligned with the pubic bone. Slowly place legs back together once the PUREWICK™ Female External Catheter is positioned.

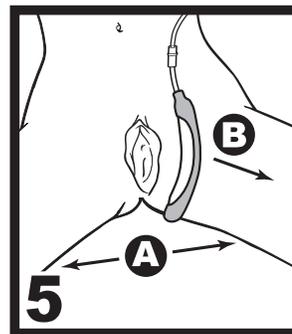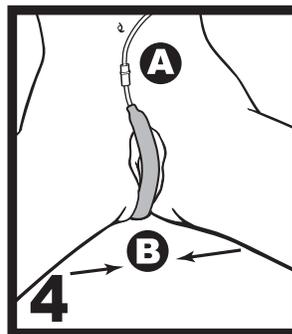

Maintenance:

6. Replace the PUREWICK™ Female External Catheter at least every 8-12 hours or if soiled with feces or blood. Always assess skin for compromise and perform perineal care prior to placement of a new PUREWICK™ Female External Catheter.

Note: Patient can be positioned on back, side lying, frog legged, or lying on back with knees bent and thighs apart (lithotomy position) prior to device placement.

Removal:


5. To remove the PUREWICK™ Female External Catheter, fully separate the legs, gluteus, and labia. To avoid potential skin injury upon removal, gently pull the PUREWICK™ Female External Catheter directly outward. Ensure suction is maintained while removing the PUREWICK™ Female External Catheter. After use, this product may be a potential biohazard. Dispose of in accordance with applicable local, state and federal laws and regulations.

Attach to hospital wall suction or DRYDOC™ Vacuum Station suction

Align with pubic bone

Place gauze facing patient

Tuck between gluteus

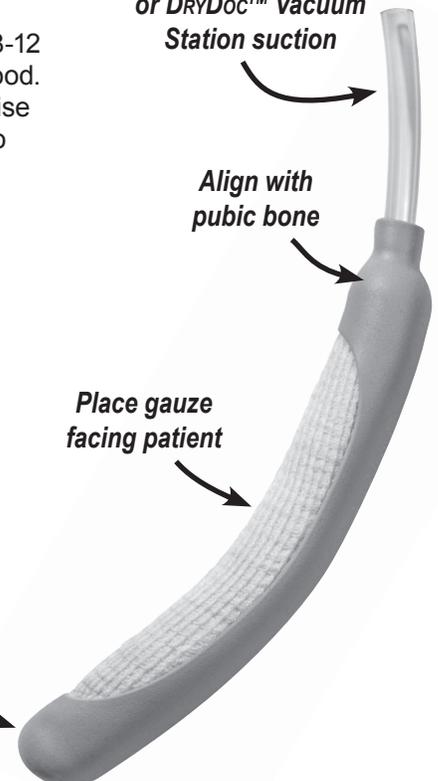

PUREWICK™

FEMALE EXTERNAL CATHETER

Indication for use:

The PUREWICK™ Female External Catheter is intended for non-invasive urine output management in female patients.

EXTERNAL USE ONLY

Caution: This Product Contains Dry Natural Rubber

Contraindications:

- Patients with urinary retention

Warnings:

- Do not use the PUREWICK™ Female External Catheter with bedpan or any material that does not allow for sufficient airflow.
- To avoid potential skin injury, never push or pull the PUREWICK™ Female External Catheter against the skin during placement or removal.
- Never insert the PUREWICK™ Female External Catheter into vagina, anal canal, or other body cavities.
- Discontinue use if an allergic reaction occurs.
- After use, this product may be a potential biohazard. Dispose of in accordance with applicable local, state and federal laws and regulations.

Precautions:

- Not recommended for patients who are:
 - Agitated, combative, or uncooperative and might remove the PUREWICK™ Female External Catheter
 - Having frequent episodes of bowel incontinence without a fecal management system in place
 - Experiencing skin irritation or breakdown at the site
 - Experiencing moderate/heavy menstruation and cannot use a tampon
- Do not use barrier cream on the perineum when using the PUREWICK™ Female External Catheter. Barrier cream may impede suction.
- Not recommended for use on patients with a known latex allergy.
- Proceed with caution in patients who have undergone recent surgery of the external urogenital tract.
- Always assess skin for compromise and perform perineal care prior to placement of a new PUREWICK™ Female External Catheter.
- Maintain suction until the PUREWICK™ Female External Catheter is fully removed from the patient to avoid urine backflow.

Recommendations:

- Perform each step with clean technique. In the home setting, wash hands thoroughly before device placement.
- Prior to connecting the PUREWICK™ Female External Catheter to hospital wall suction tubing, verify suction function by covering the open end of the suction tubing with one hand and observing the pressure dial. If the pressure does not increase when the line is covered, verify that the tubing is secured, connected, and not kinked.
- Ensure the PUREWICK™ Female External Catheter remains in the correct position after turning the patient. Remove the PUREWICK™ Female External Catheter prior to ambulation.
- Properly placing the PUREWICK™ Female External Catheter snugly between the labia and gluteus holds the PUREWICK™ Female External Catheter in place for most patients. Mesh underwear may be useful for securing the PUREWICK™ Female External Catheter for some patients.
- Assess device placement and patient's skin at least every 2 hours.
- Replace the PUREWICK™ Female External Catheter every 8-12 hours or when soiled with feces or blood.
- Change suction tubing per hospital protocol or at least every thirty (30) days.

 Units	This Product Contains Dry Natural Rubber
 Single Use	 Non-sterile
 Catalog number	 Do not use if package is damaged
 Lot number	 Use by date

 Manufacturer:
C. R. Bard, Inc.
Covington, GA 30014 USA
1-800-526-4455
www.purewick.com

Bard, DryDoc, and PureWick are trademarks and/or registered trademarks of C. R. Bard, Inc.
Copyright © 2018 C. R. Bard, Inc. All Rights Reserved.

